


Amplification:

Before starting the amplification:

- ✓ The addition of the enzyme mix should be done with a pipette in the range of 1-2 µl.
- ✓ Keep the amplification tubes at 4°C at all times.

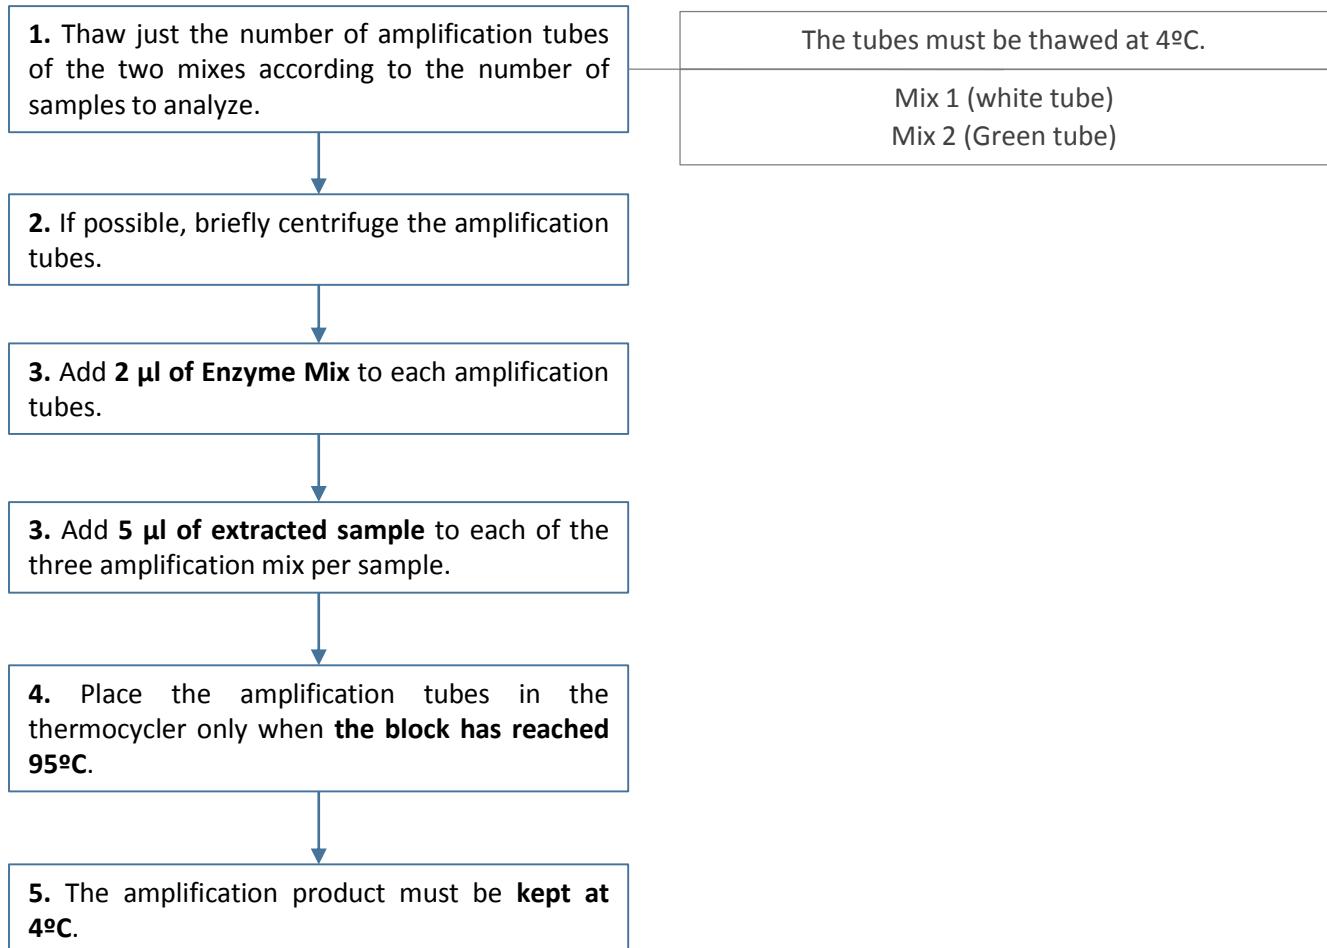

PCR program:

1 cycle	45°C	45'
	95°C	15'
45 cycles	95°C	30"
	50°C	1'30"
	68°C	1'
1 cycle	68°C	10'
1 cycle	4°C	∞