


## Amplification:

Before starting the amplification:

- ✓ The extraction product must have a minimal DNA/RNA concentration of 5-10 ng/µl.
- ✓ The addition of the enzyme mix should be done with a pipette in the range of 1-2 µl.
- ✓ Keep the amplification tubes at 4°C at all times.

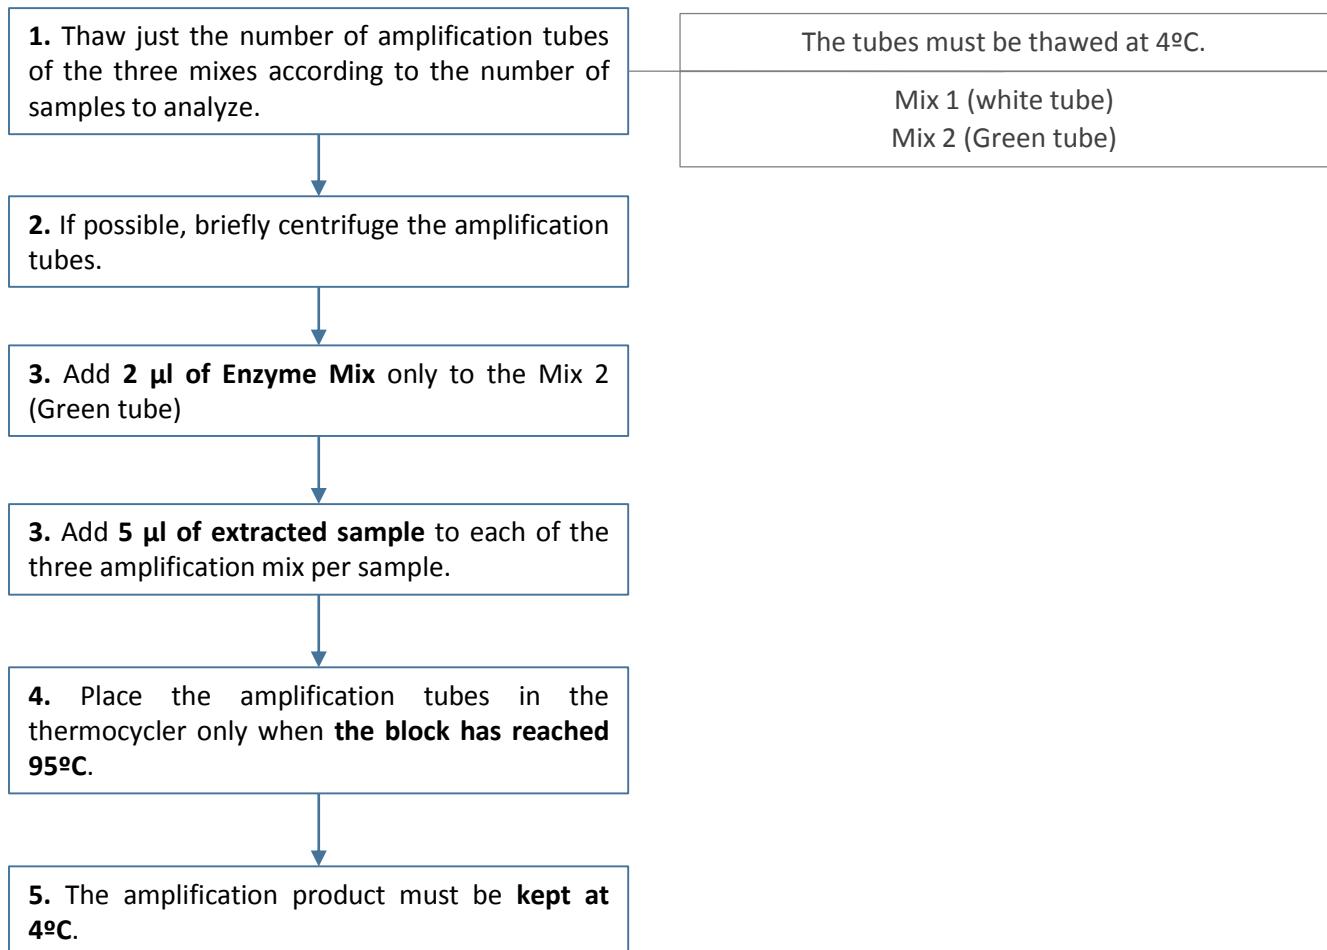

**PCR program:**

<b>1 cycle</b>	45°C	45'
	95°C	15'
<b>45 cycles</b>	95°C	30"
	56°C	1'30"
	72°C	1'
<b>1 cycle</b>	72°C	10'
<b>1 cycle</b>	4°C	∞